


REV	DESCRIPTION	DRN	CHK	APP	DATE
0	INITIAL RELEASE	JY			09/10

THE DRAWINGS, SPECIFICATIONS AND OTHER DATA HEREIN PROVIDED SHALL NOT BE COPIED, PUBLISHED OR OTHERWISE FURTHER DISSEMINATED WITHOUT PRIOR WRITTEN PERMISSION OF STANFORD UNIVERSITY / SLAC.

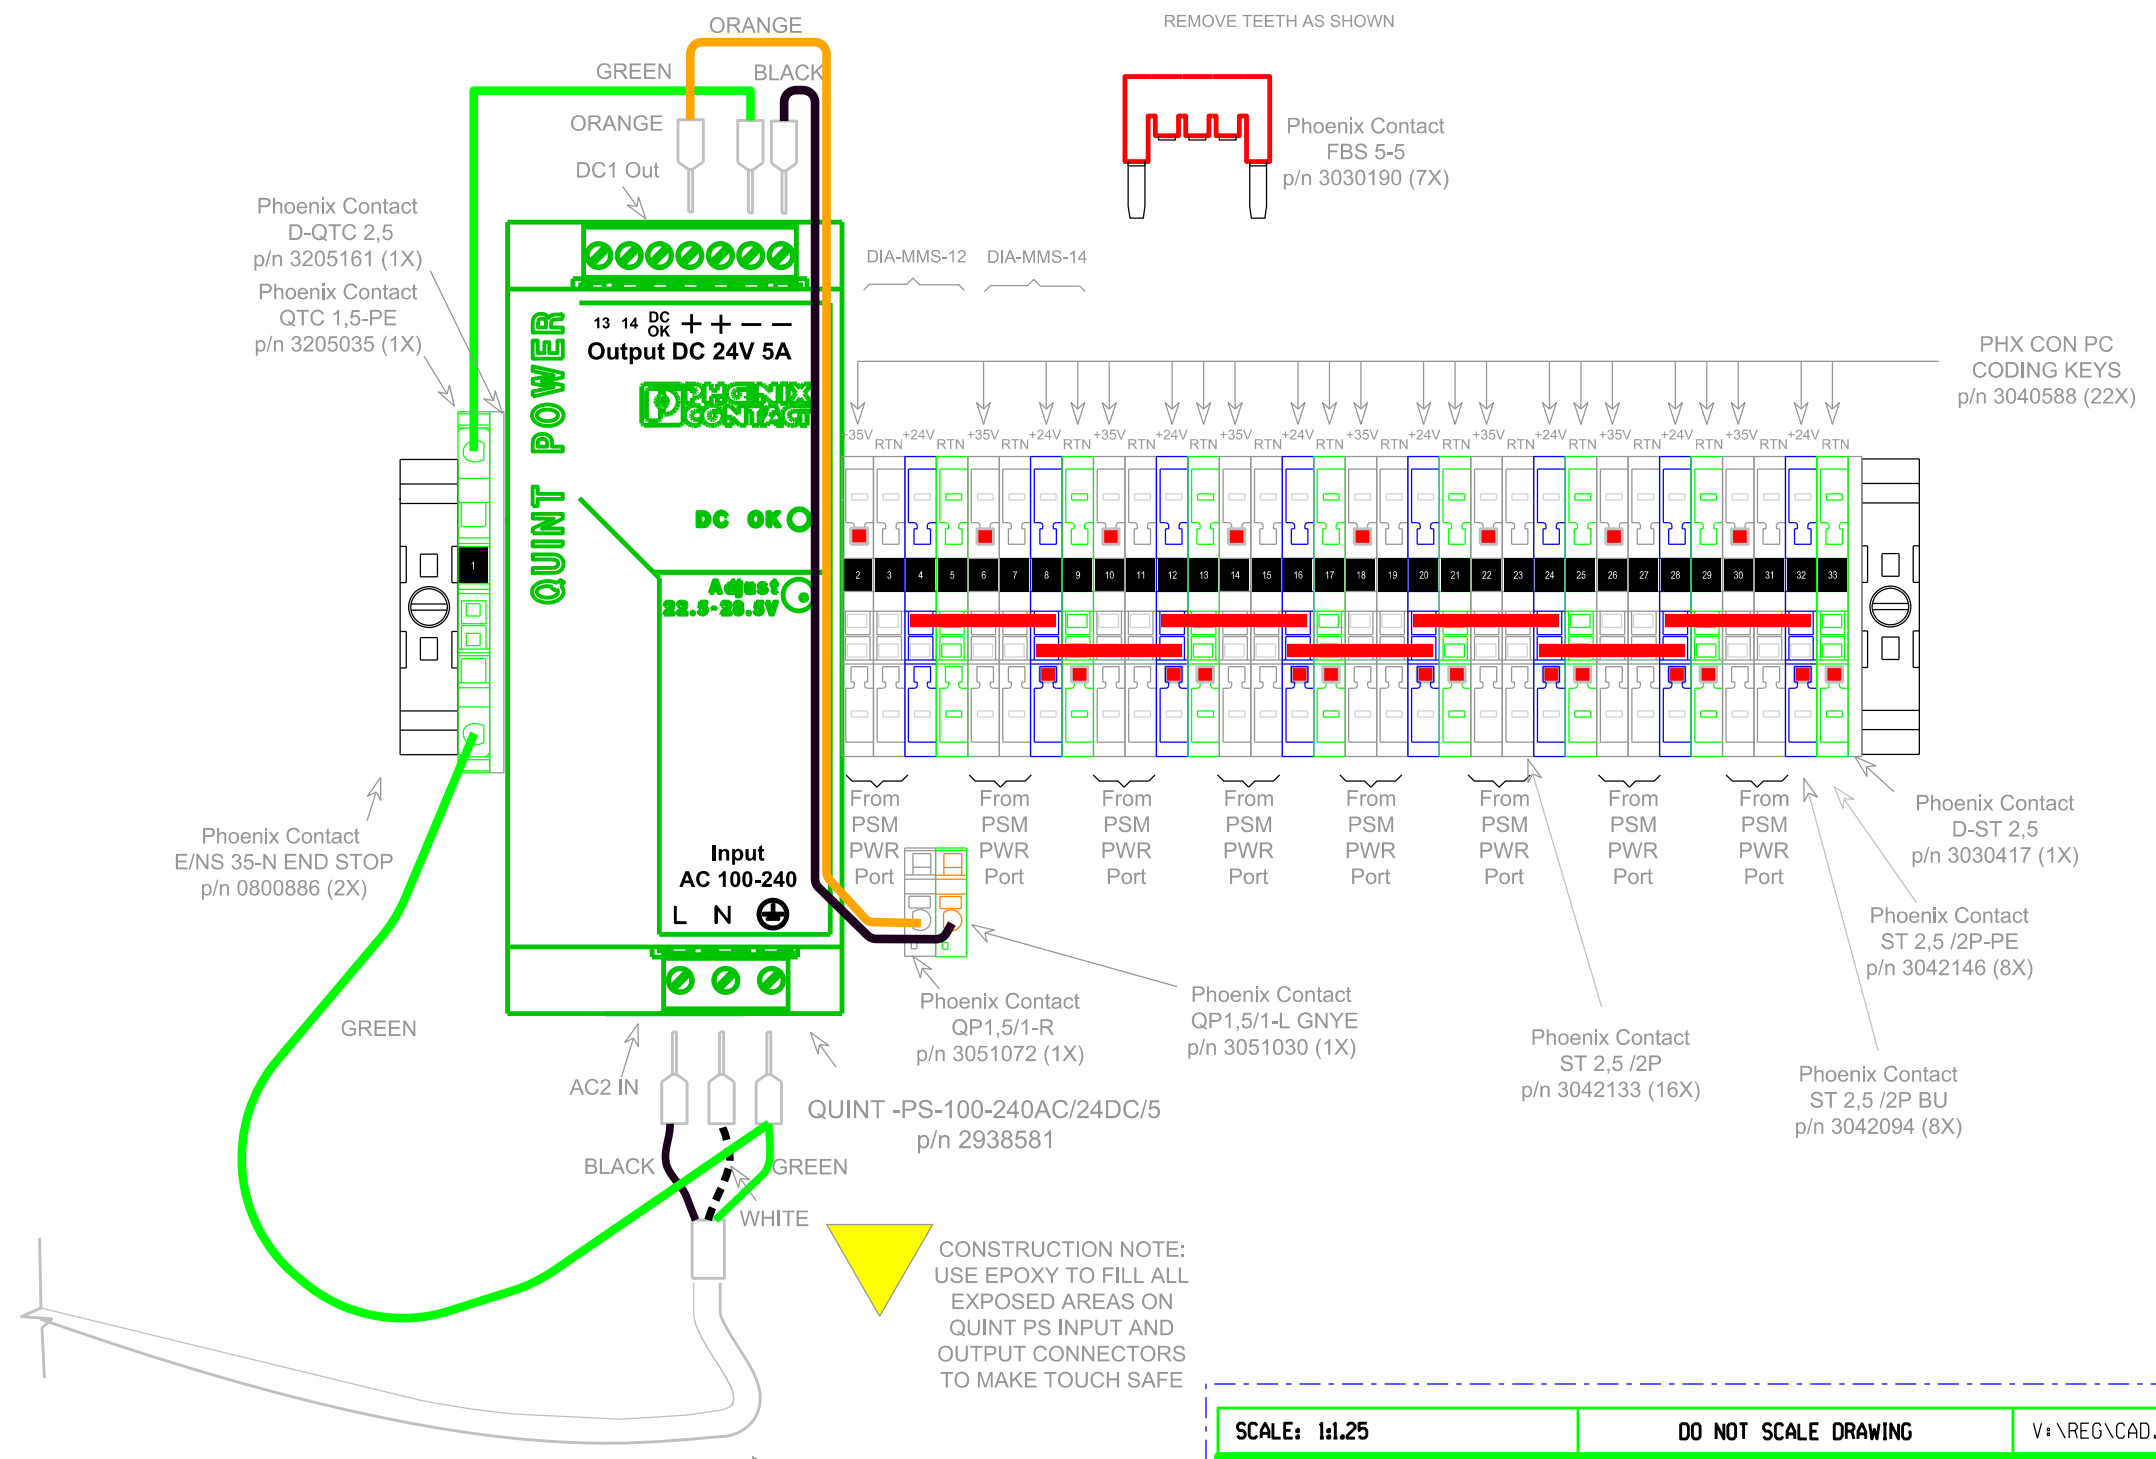

**CONSTRUCTION NOTE:**  
Unless otherwise specified, all cables are to be stranded 18AWG wires with applicable ferrules crimped on the end.

18AWG ELECTRIC CORD (TYPICAL LENGTH = 2 METERS)

**CONSTRUCTION NOTE:**  
USE EPOXY TO FILL ALL EXPOSED AREAS ON QUINT PS INPUT AND OUTPUT CONNECTORS TO MAKE TOUCH SAFE

SCALE: 1:1.25	DO NOT SCALE DRAWING	V:\REG\CAD...\CXI\DN...\CXI-XR50-DRL-21.DGN	1 OF 1
		LCLS PCD SYSTEMS CXI PARKER BRAKE PWR CXI-XR50-DRL-21	
ENGR _____	DATE 09/01/10	APPROVALS _____	
DRTS J.YIN			
CHKD _____			
AD 261-600-41			B