



# Cryogenic Power over Fiber for fundamental and applied physics at Milano Bicocca

*Marta Torti*

*Istituto Nazionale di Fisica Nucleare – Sezione di Milano Bicocca*

**TIPP2023**

**TECHNOLOGY IN INSTRUMENTATION &  
PARTICLE PHYSICS CONFERENCE**

4 - 8 SEPTEMBER 2023



Istituto Nazionale di Fisica Nucleare




- **Cryo-PoF:** Cryogenic Power over Fiber.
- It is funded by “Young Researcher Grant” from Istituto Nazionale di Fisica Nucleare (INFN, Italy) (INFN CSN5 Young Grant 2021) from February 2022 for 2 years; PI: M. Torti; Institutions: Univ. Milano-Bicocca and Univ. Milano Statale.
- **Cryo-PoF’s main goal** is to power, at cryogenic temperature, both SiPM and cold amplifier, using a single Power over Fiber line and to tune SiPM bias with the laser power.
- In this talk:
  - Cryo-PoF idea and setup;
  - results and comparison with the copper cable results in LN;
  - preliminary test at lower temperature ( $\sim 10$  K).

- The **Power over Fiber** (PoF) technology delivers electrical power by sending laser light, through an optical fiber, to a photovoltaic power converter, in order to power sensors or electrical devices.
- Several producers of PoF systems are available on the market and this technology has been already employed in industry.
- No attempt has been done to port the technique at the cryogenic level. The reason is that electronic components are certified down to 233 K ( $-40^{\circ}$  C) .
- PoF solution offers several **advantages**:
  - removal of noise induced by standard power lines,
  - robustness in a hostile environment,
  - spark free operation when electric fields are present,
  - no interference with electromagnetic fields.
- Ideal solution where the environmental conditions are prohibitive for a copper-based power line.


# DUNE Vertical Drift

- **DUNE Vertical Drift (VD) module:** LAr TPC in which electrons drift toward the anodes placed on top and bottom of the detector. Anode planes will be made by PCBs, so light opaque.
- The grid cathode is at half height and operated at 320 kV.
- **Photon Detection System\*** (PDS) can be placed on the cathode or outside the field cage with much lower photon collection efficiency .
- PoF is the chosen technology to power the PDS (*W. Pellico's idea: "Power over fiber", talk at the DUNE FD-2 (VD) Photon Detector Workshop, Jul 26-27 2021, <https://indico.fnal.gov/event/50157/> )*

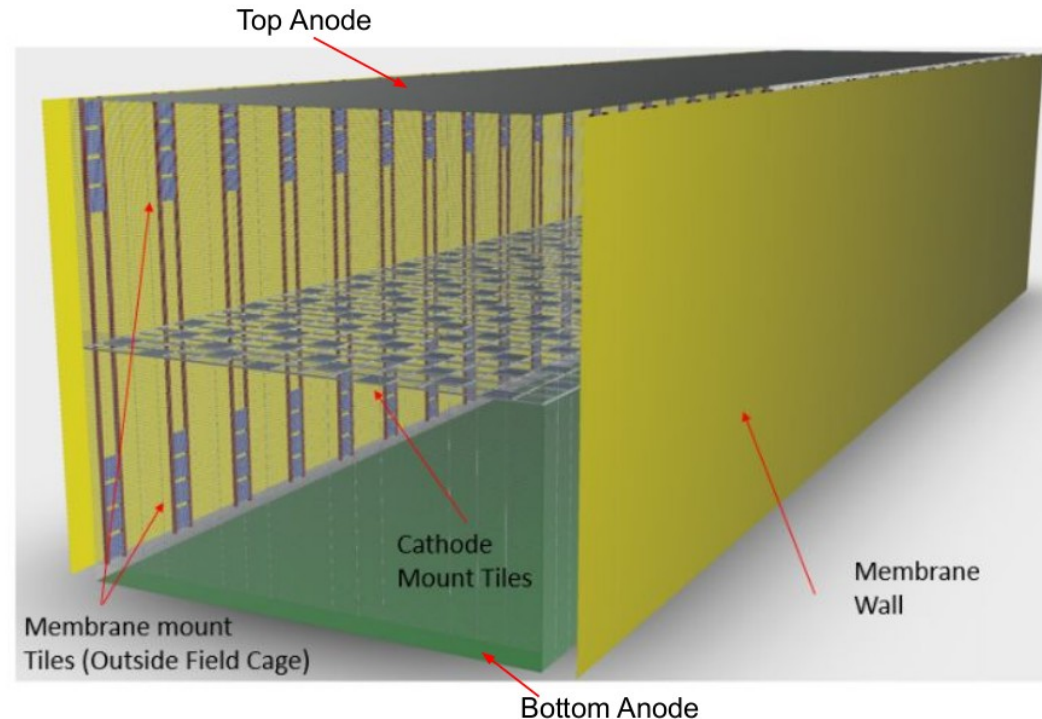

\* see *F. Di Capua's talk "Photon Detection System in the far detector module of the DUNE experiment"* for details.

# Cryo-PoF : the concept

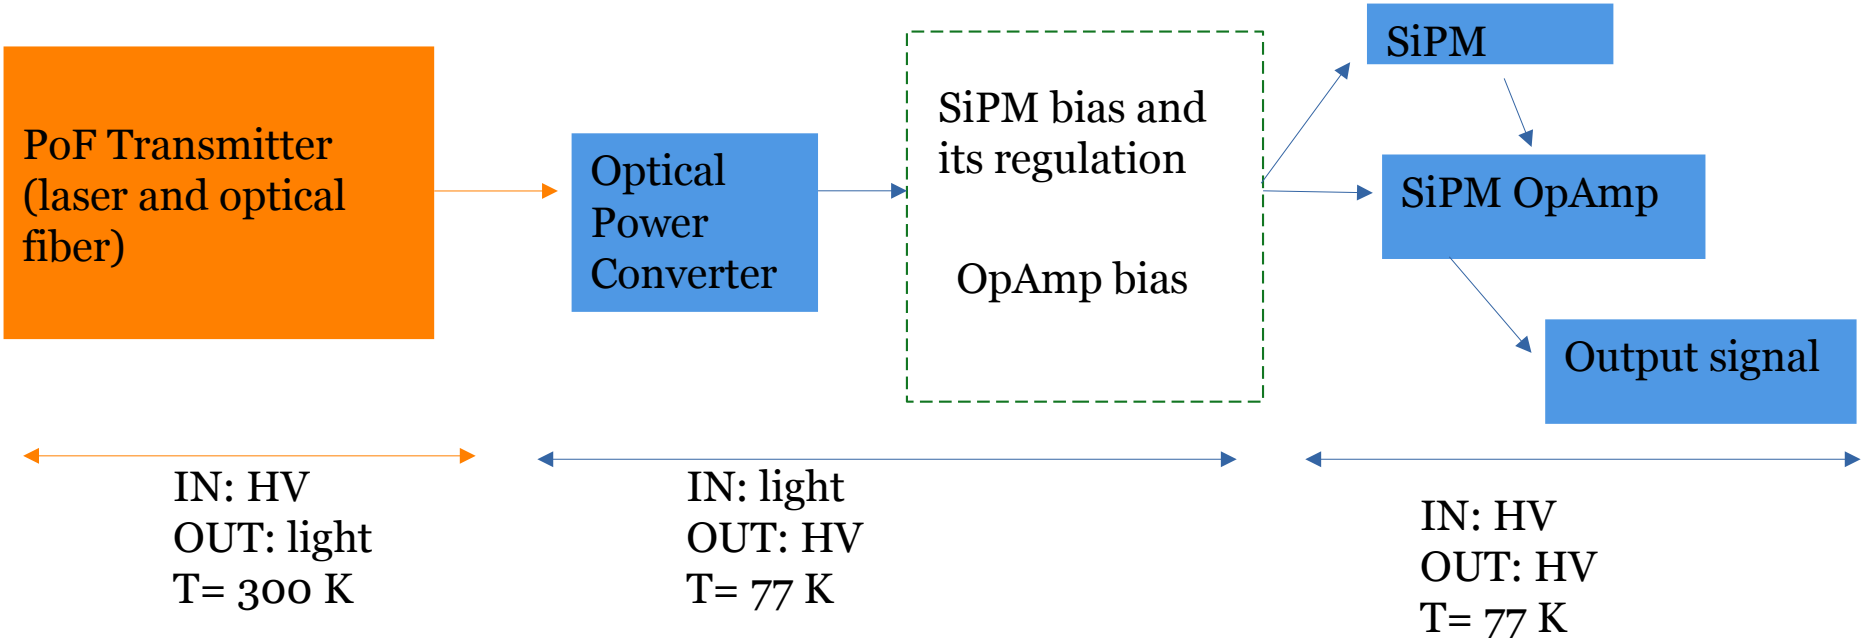

# Laser source




- **GaAs laser source:** 808 nm

*Why?*




SiPMs photon detection efficiency has a peak around 500 nm

→ laser light should better be far from it!

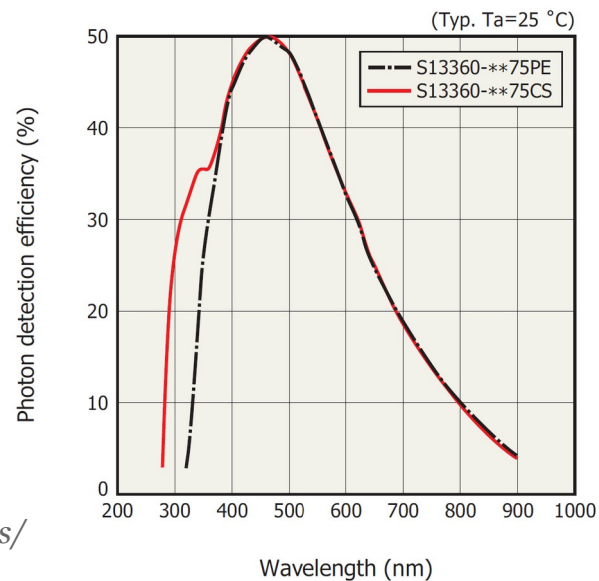


# Laser source


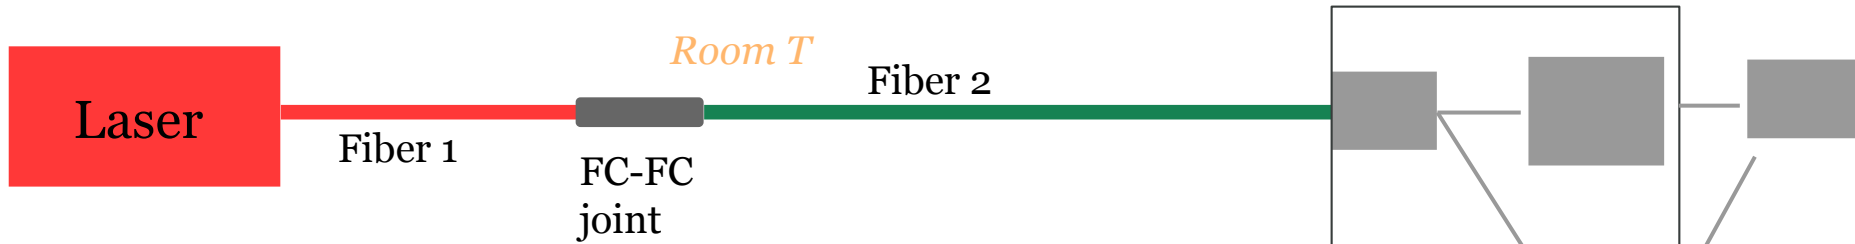


- **GaAs laser source**, 808 nm AFBR-POMEK2204 Broadcom, directly connected to a multimode optical fiber (62.5  $\mu\text{m}$  core diameter).
- Characterization of the laser source in terms of:
  - linearity,
  - power loss connecting an **optical fiber**,
  - stability over time.


**Graded index multi mode optical fiber** (core diameter 62.5  $\mu\text{m}$ ) with 6.1 mm Stainless Steel tubing with black plastic sheath, from Thorlabs

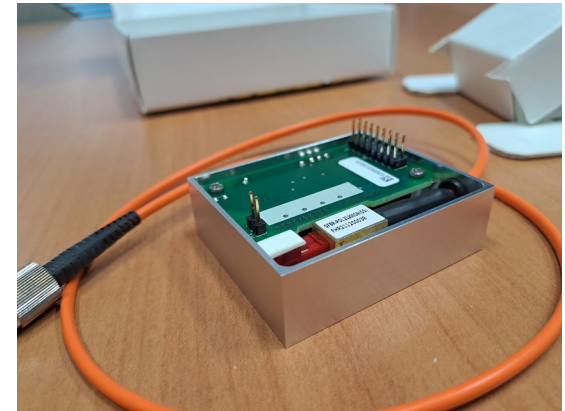

# Laser source

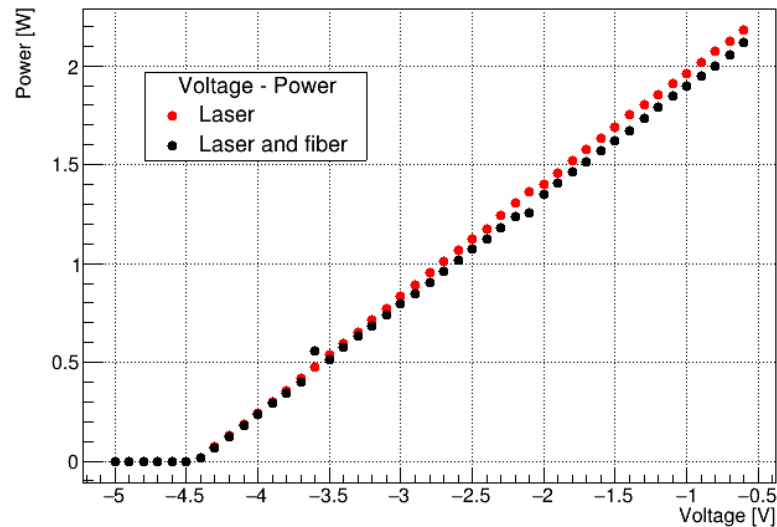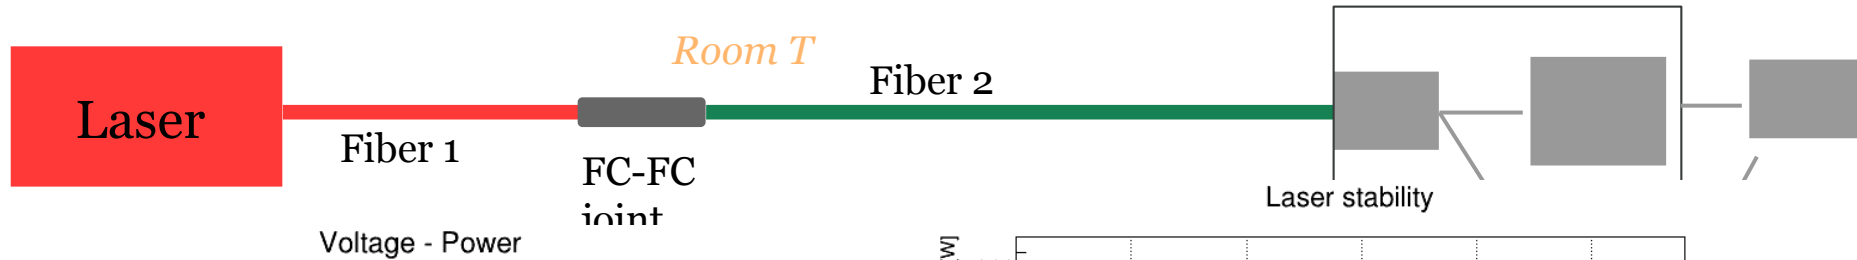

~ 4.5 % power loss adding a FC/FC joint and an optical fiber.

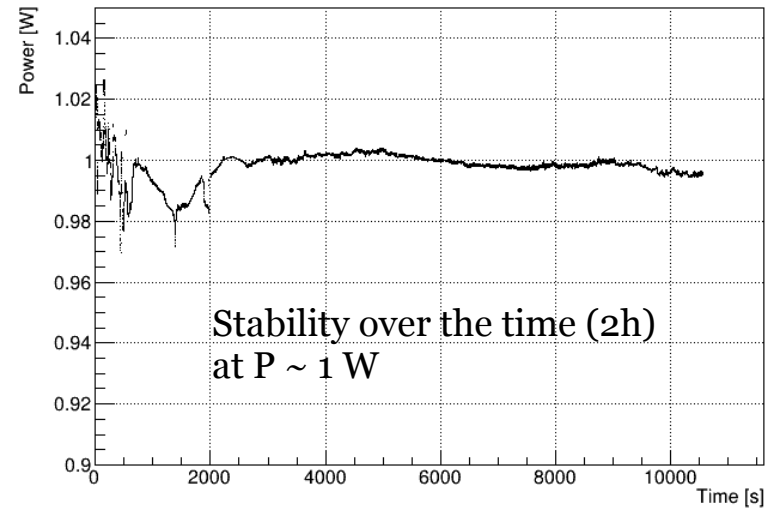



Max - Min ~ 5.7% - Mean( $P_o - P_i$ ) = 17.1 mW

Without the first 30 min:

Max - Min ~ 0.96% - Mean( $P_o - P_i$ ) = 15.9 mW



# Optical Power Converter

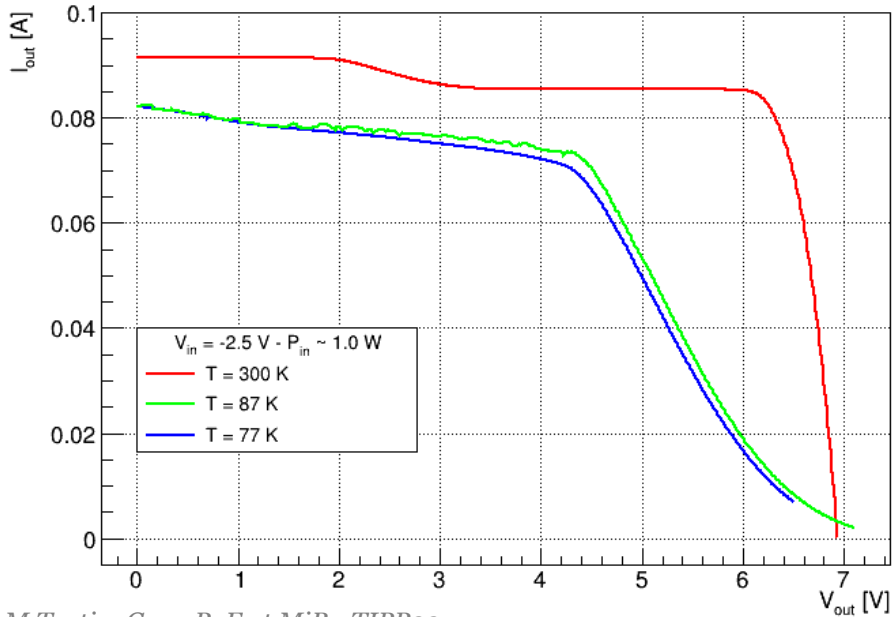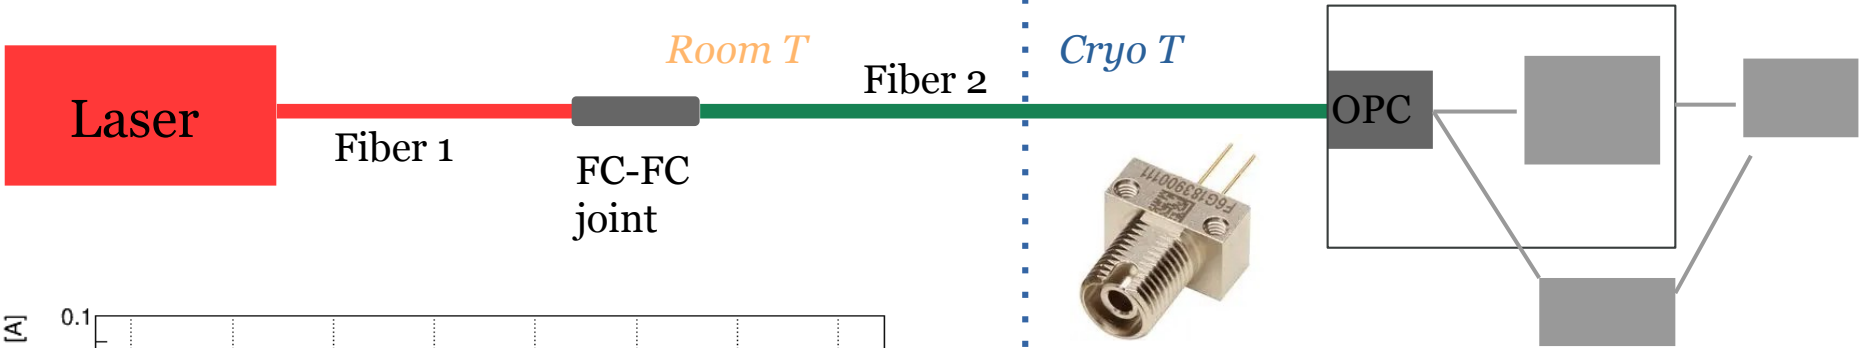

- Optical power converter, AFBR-POC206L from Broadcom
- IV curves using a semiconductor analyser
- Tested at different  $P_{in}$



$P_{in} \sim 1 W$

$T = 300 K : P_{max} = 0.52 W, I_{max} = 91.4 mA$


$T = 87 K : P_{max} = 0.32 W, I_{max} = 82.5 mA$

$T = 77 K : P_{max} = 0.30 W, I_{max} = 82.2 mA$



# From laser to SiPM

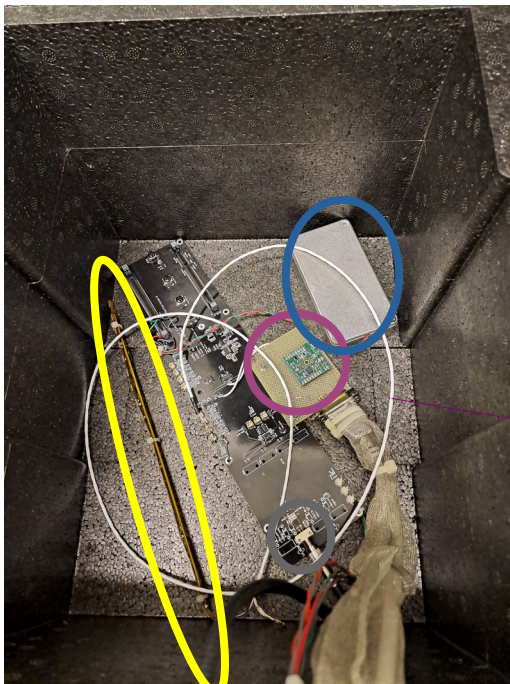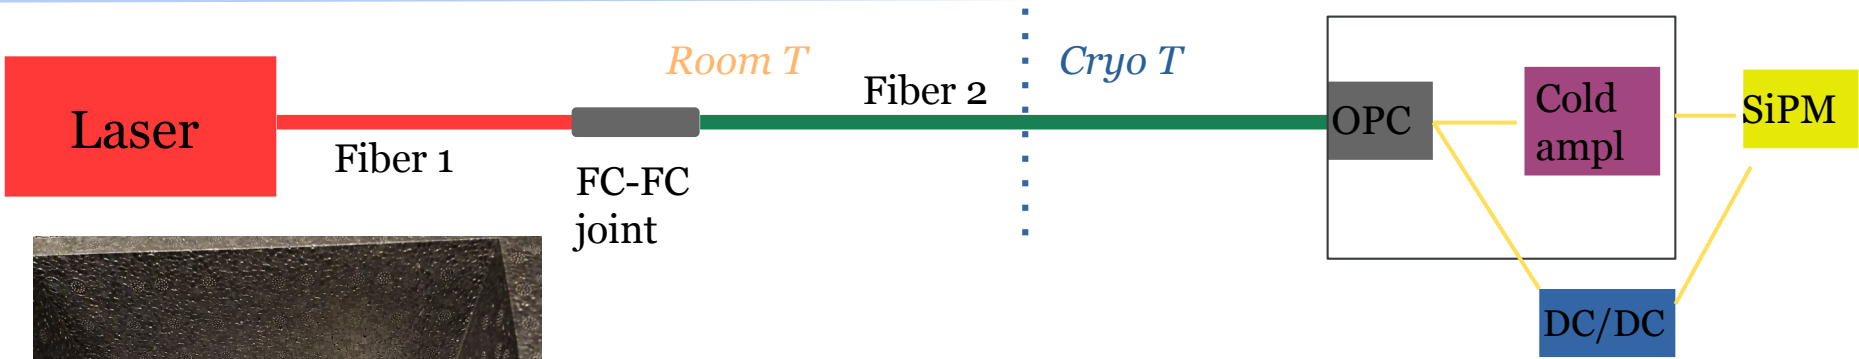


- **Cold amplifier** developed by Milano Bicocca group for DUNE,  
 $\rightarrow V_{in} = 3.3 V$

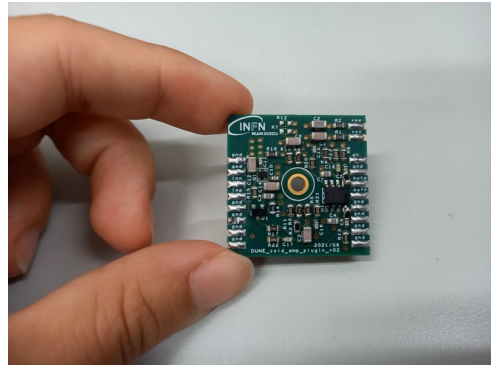

# From laser to SiPM

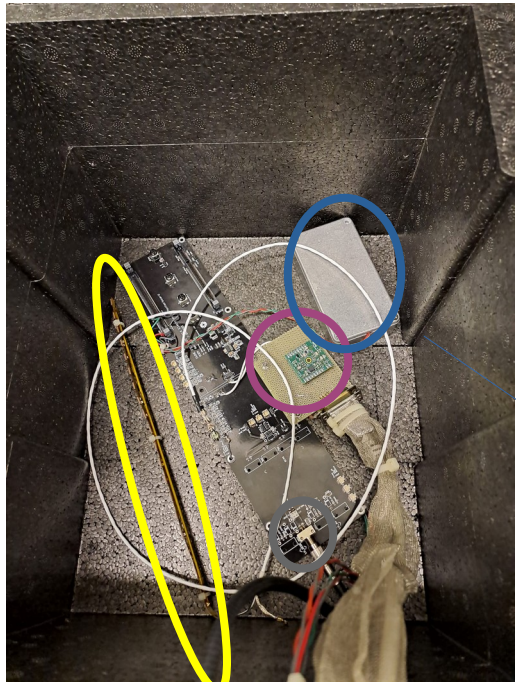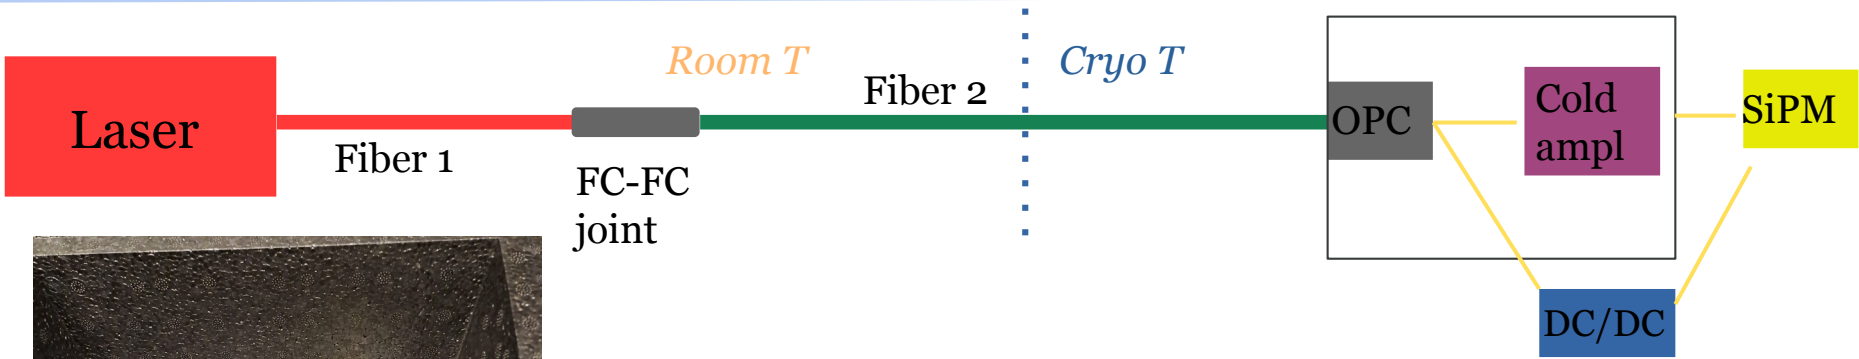


- **DC/DC** boost converter developed by INFN Milano Statale group,
  - $V_{in} \sim 5\text{ V}$ ;  $V_{out} \sim [40, 50]\text{ V}$ ,
  - give bias to SiPMs;
  - placed in a metallic box to reduce noise. *Work in progress!*

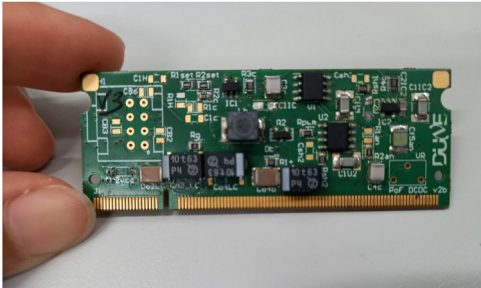

[https://indico.fnal.gov/event/54005/contributions/238717/attachments/154042/200047/Workshop\\_BNL\\_13\\_04\\_2022.pptx-1.pdf](https://indico.fnal.gov/event/54005/contributions/238717/attachments/154042/200047/Workshop_BNL_13_04_2022.pptx-1.pdf)

# DC/DC boost converter


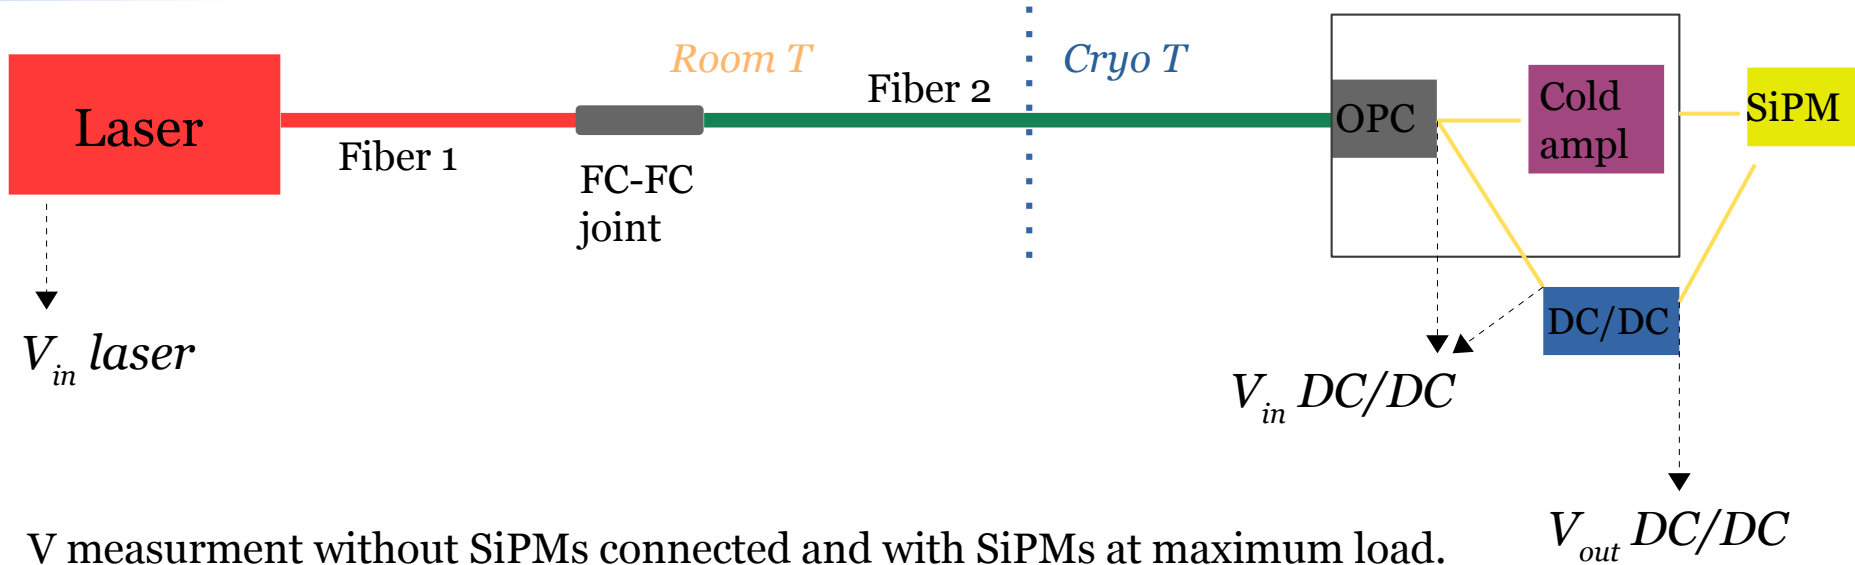


$V_{in \text{ laser}}$  → V laser source input, proportional to the laser power;


$V_{in \text{ DC/DC}}$  → V output from the OPC, that is the DC/DC input ;

$V_{out \text{ DC/DC}}$  → V output from the DC/DC, that is the SiPMs bias voltage.

# DC/DC boost converter

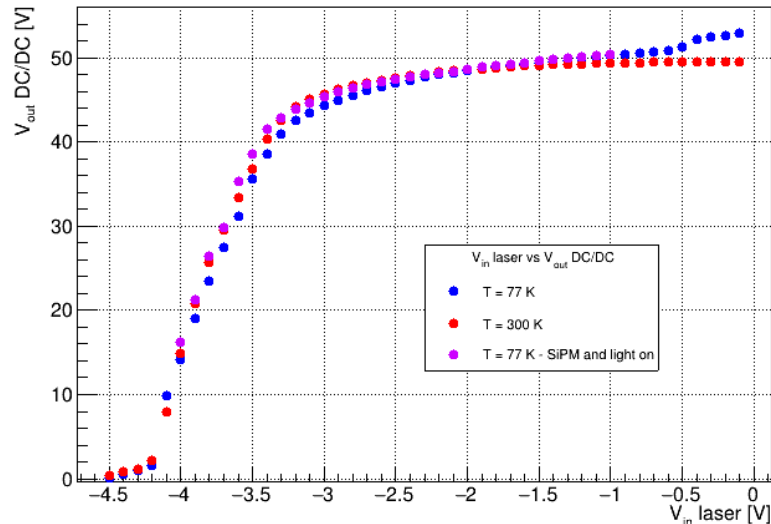
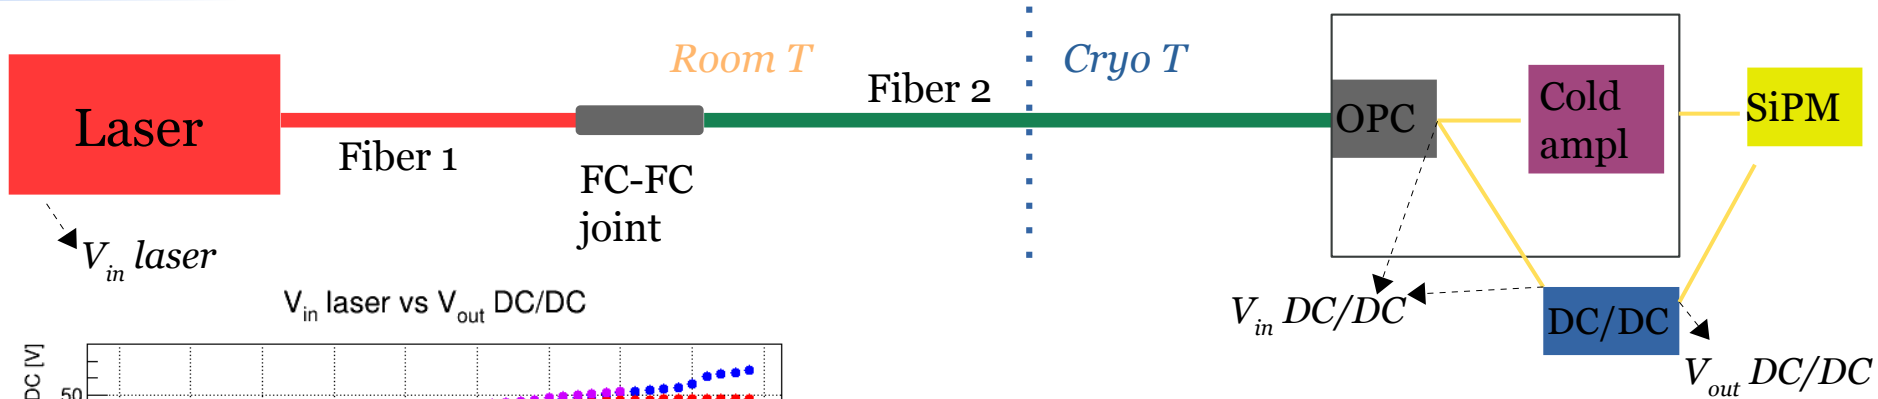


$V_{out\ DC/DC}$  increases as a function of  $V_{in\ laser}$ .

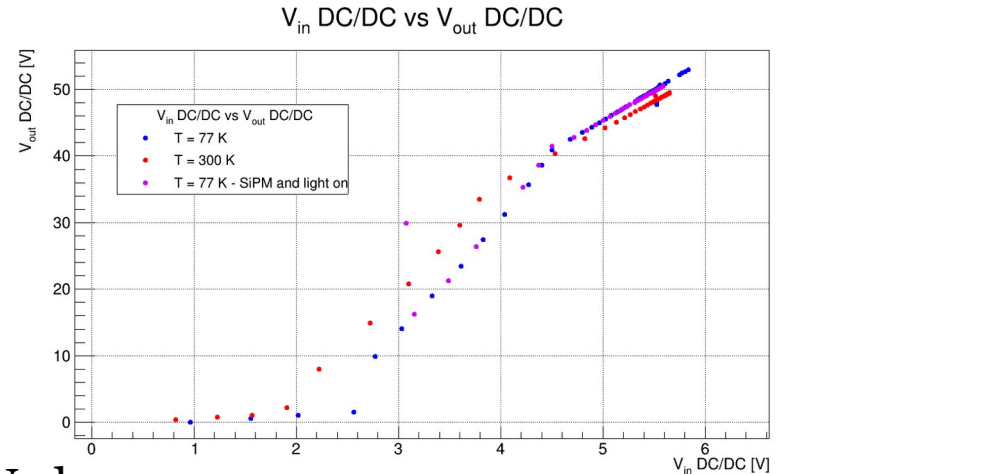




# From laser to SiPM

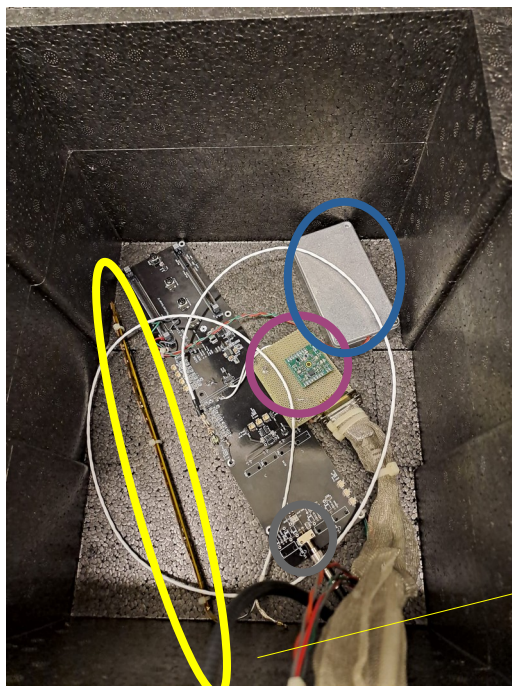
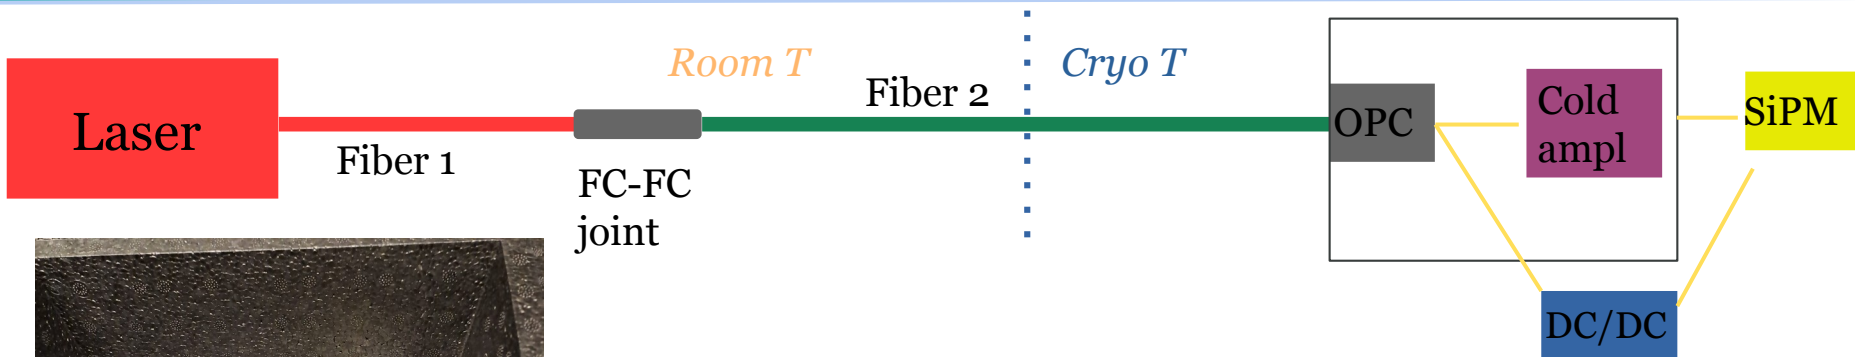


- **Hamamatsu SiPM**, developed by Hamamatsu for DUNE,
  - 1 flexi board with **20 SiPMs** in parallel,
  - $V_{bd} = 42 \text{ V}$  at 77 K.

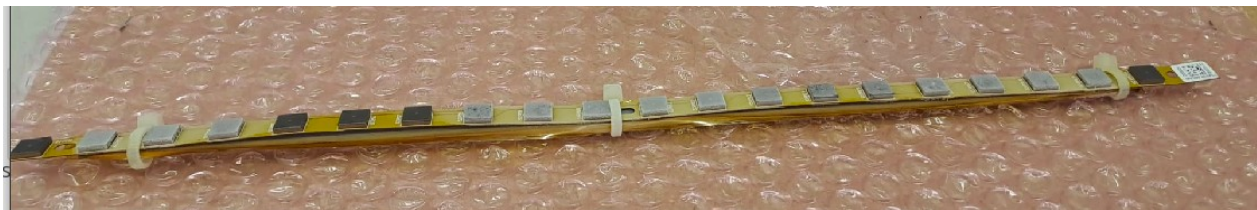

see *A.Falcone's talk "Cryogenic SiPMs for the DUNE experiment"* for details!


# From laser to SiPM - Results

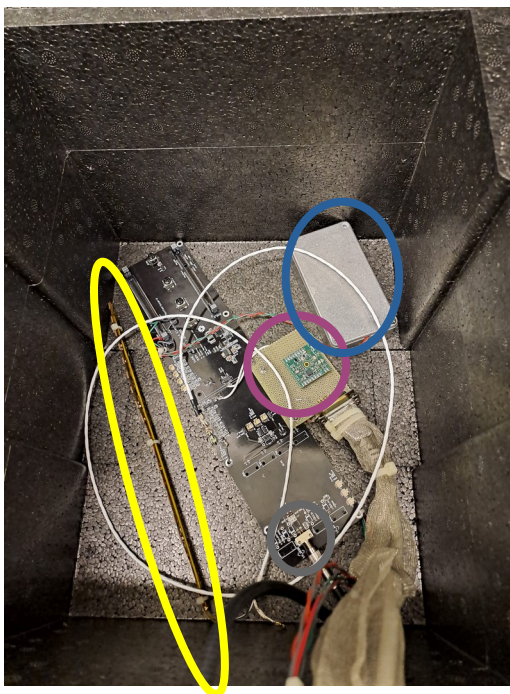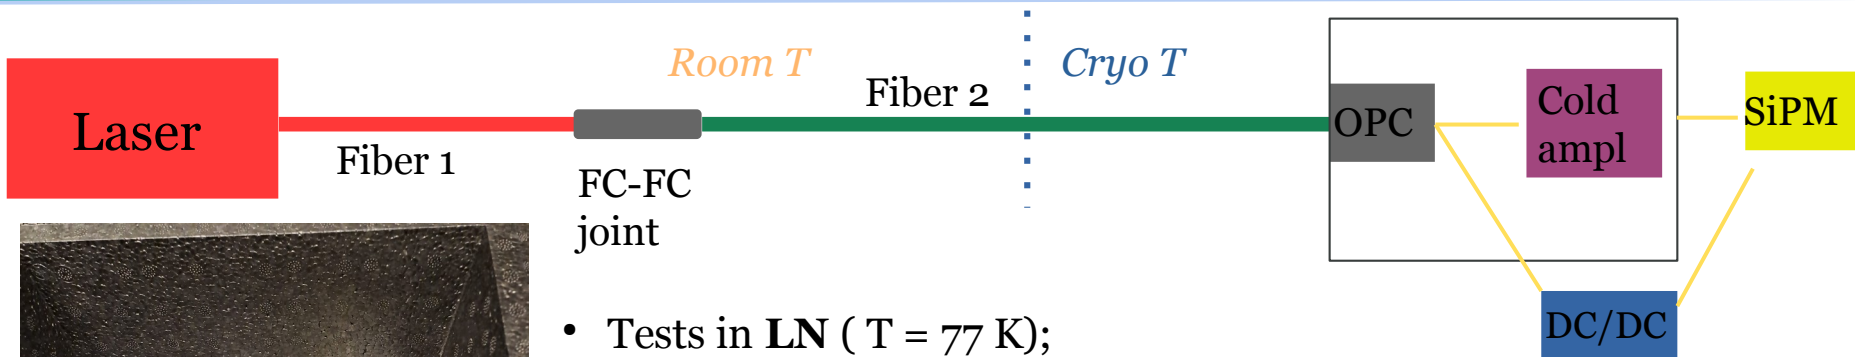

- Tests in **LN** ( $T = 77$  K);
- **20 SiPMs** in parallel ( 1 flexi board);
- **three SiPM bias** tested : 45 V, 46 V, 47 V (3, 4, 5 V ov);
- evaluation of the **Signal to Noise Ratio** (SNR);
- comparison of the results: PoF vs copper line.





# From laser to SiPM – PoF Results

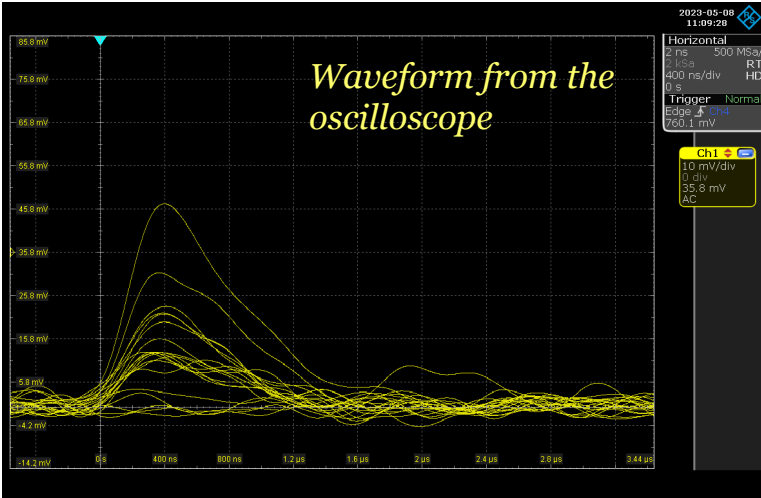

$$V_{in \text{ laser}} = -2.83 \text{ V}$$


$$V_{bias} = 46 \text{ V} - 4 \text{ V ov}$$

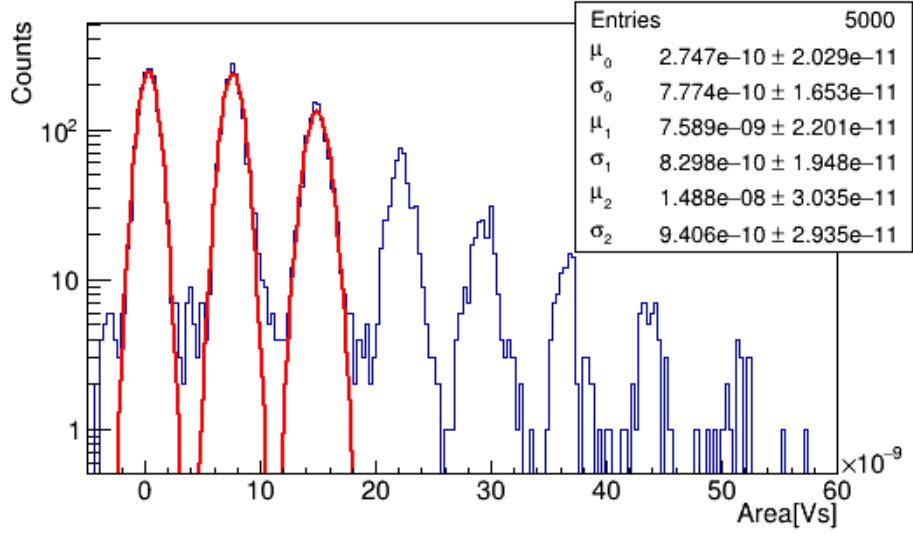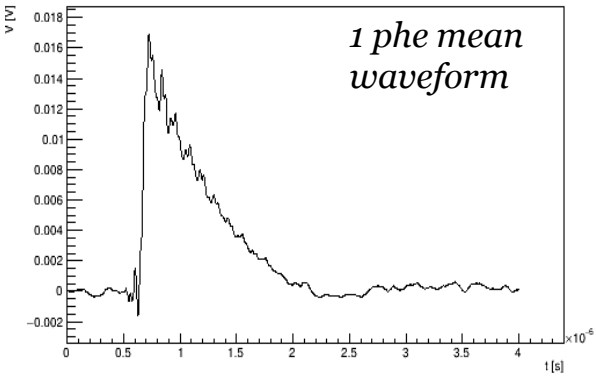

SNR = 9.409




# PoF vs copper cable

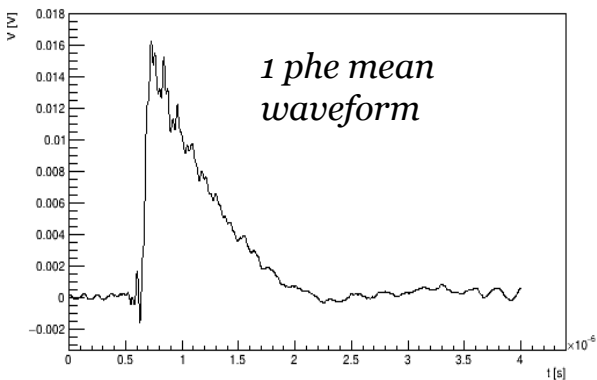

## Copper cable

$$V_{\text{bias}} = 46 \text{ V} - 4 \text{ V ov}$$

$$\text{SNR} = 10.665$$


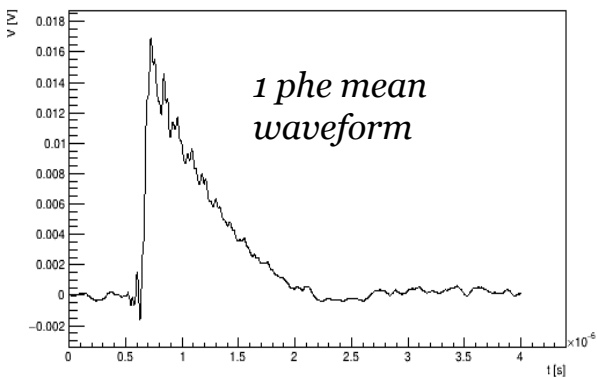


## PoF

$$V_{\text{in laser}} = -2.83 \text{ V}$$

$$V_{\text{bias}} = 46 \text{ V} - 4 \text{ V ov}$$

$$\text{SNR} = 9.409$$

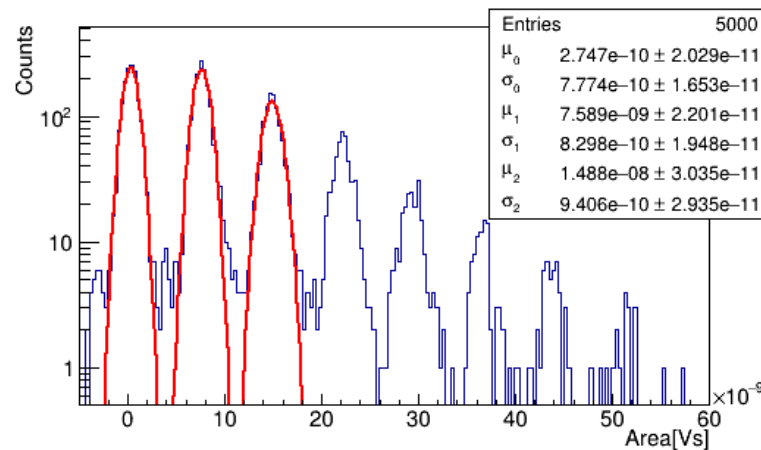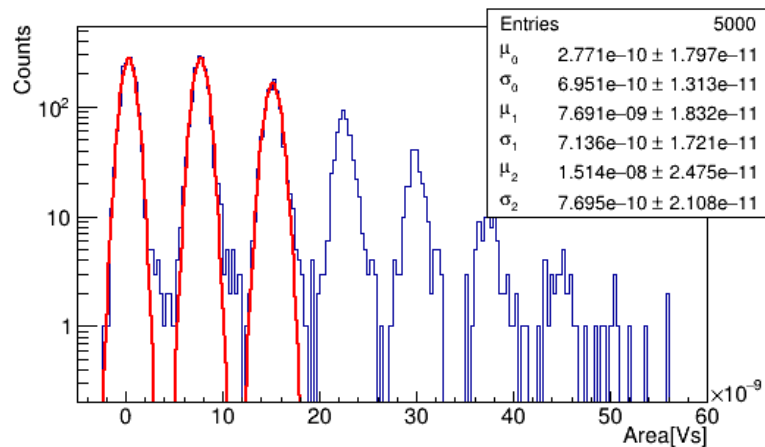


SNR is calculated for each SiPM bias tested.

		SNR	
SiPM bias	Overvoltage	<i>Copper cable</i>	<i>PoF</i>
45 V	3 V	7.830	7.520
46 V	4 V	10.665	9.409
47 V	5 V	13.004	11.070


The performances of the PoF are comparable with the copper cable ones.  
The residual noise from DC/DC will be improved: new DC/DC version is under way.

- Test Power over Fiber technology at temperature lower than 77 K.
- We tested our setup (from laser to OPC) in a cryostat **till 7 K** and characterized the OPC output registering the I-V curves with the semiconductor analyzer.
- The system was in vacuum; the temperature was fixed and controlled by means of an heater and a thermometer.
- There was a large power loss in the feedthrough (its core diameter smaller than the fiber core).
- The laser power at the OPC was  $\sim 5$  mW.


# Test at lower temperatures than LN ( $< 77$ K) - Setup

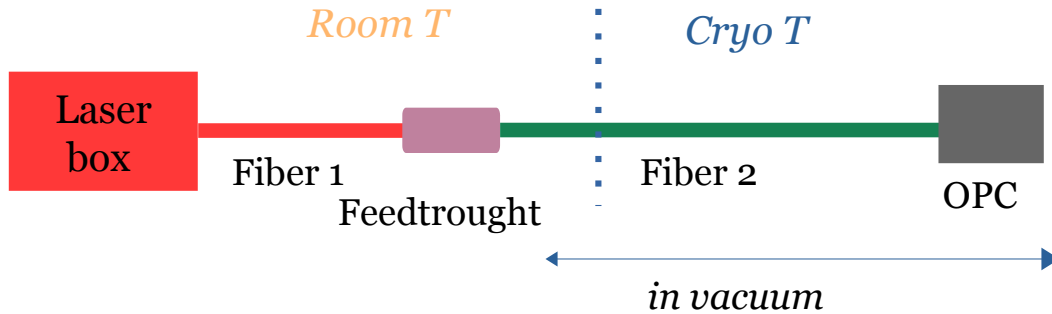


- **Laser Box** with the GaAs laser source, 808 nm;
- **optical feedtrought** (50  $\mu\text{m}$  core diameter);
- **graded index multi mode optical fiber** with 62.5  $\mu\text{m}$  core diameter;
- **optical power converter** AFBR-POC206L from Broadcom,
- temperature sensors,
- heater.

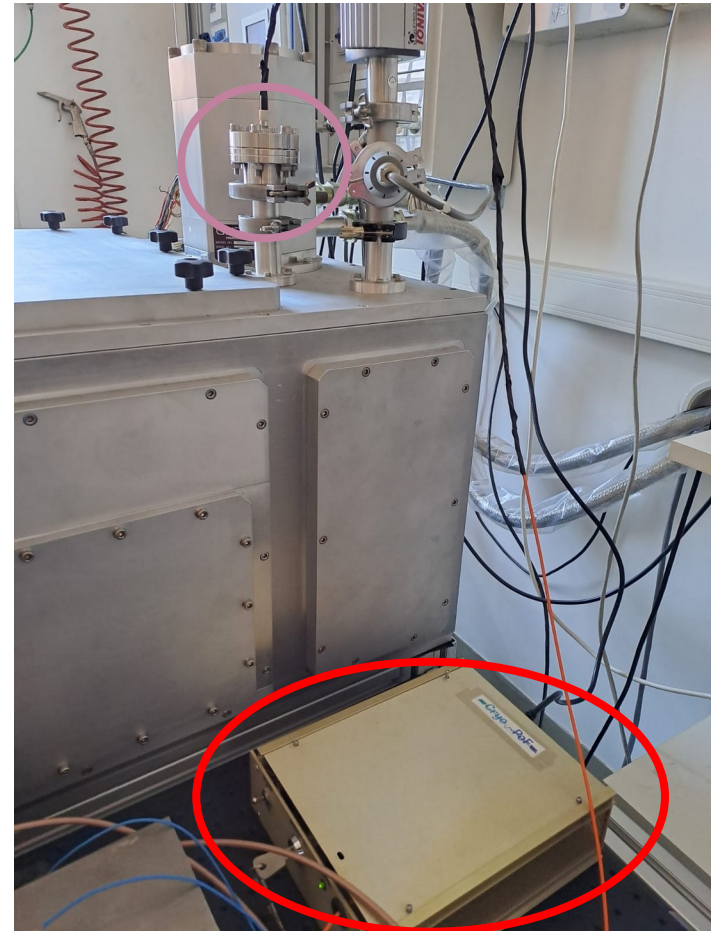


# Test at lower temperatures than LN ( $< 77$ K) - Setup

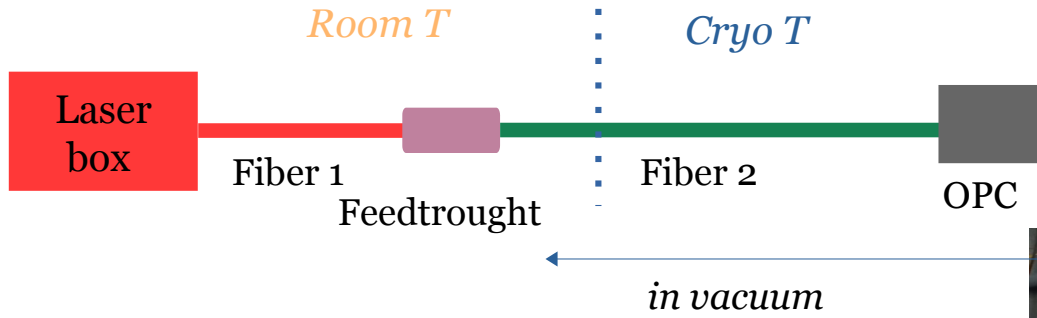

- **Laser Box** with the GaAs laser source, 808 nm;
- **optical feedtrought** (50  $\mu\text{m}$  core diameter);
- **graded index multi mode optical fiber** with 62.5  $\mu\text{m}$  core diameter;
- **optical power converter** AFBR-POC206L from Broadcom;
- **temperature sensors**;
- **heater**.

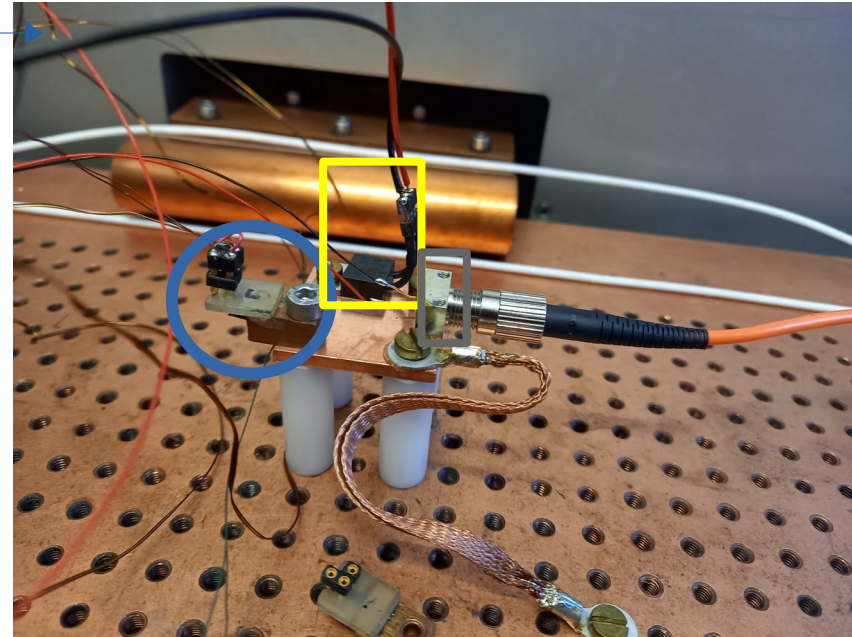

# Test at lower temperatures than LN (< 77 K) - Results

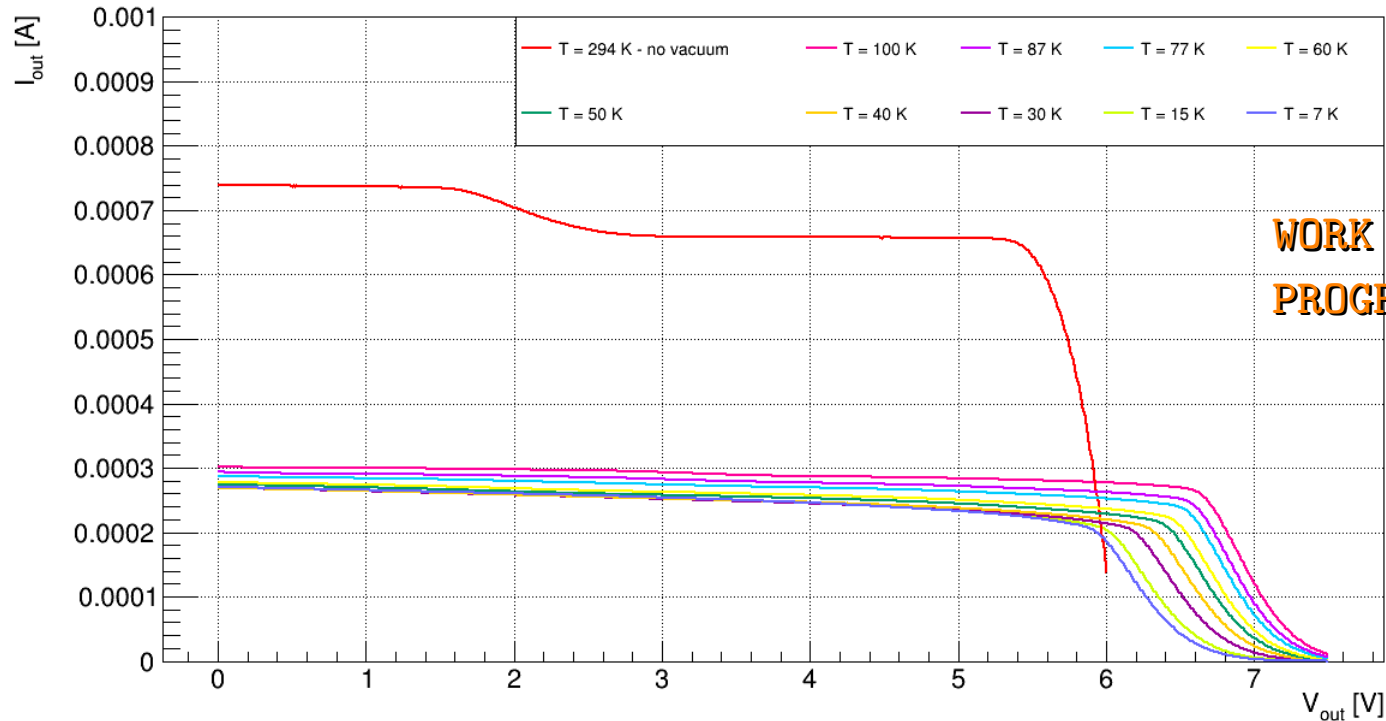

The device works till 7 K with  $P_{max} \sim 15 \% P_{in}$ .

- The main goal of Cryo-PoF is to power both SiPM and cold amplifier, using a single Power over Fiber line.
- We reach the goal and we are able to change the SiPM bias, modifying the laser power.
- Comparing the SNR of SiPMs at different overvoltages with and without PoF, we obtain good results.
- We test the PoF line at very low temperature ( till 7 K) with promising results.
- We are working to improve!

*We are grateful to the Fermilab and BNL DUNE groups, the Univ. of Milano Statale and the Univ. of Parma for support and suggestions!*

# Thank you!



Gryo-PoF






# Back up









# OPC radio purity measurements

- We performed a **gamma spectroscopy** in order to measure the radio purity of the Broadcom Optical Power Converter (AFBR-POC206L).
- A Ge detector was used.
- The live time of the measurements was 1038 h, while background measurement was taken for 321 h.
- Before this test, the device was **already soldered** to an electronic board. It has to be removed from the support and cleaned.
- The measured activities are calculated with a confidence level of 90%.
- We did not observe contaminations, with the exception of potassium, for which an excess was found.




	Activity [Bq/Kg]
$^{232}\text{Th}$	
$^{228}\text{Ac}$	<0.2
$^{208}\text{Tl}$	<0.3
$^{238}\text{U}$	
$^{226}\text{Ra}$	<2
$^{214}\text{Bi}$	<0.2
$^{235}\text{U}$	<0.1
$^{40}\text{K}$	$15 \pm 2$
$^{60}\text{Co}$	<0.07
$^{137}\text{Cs}$	<0.06

Waveform from the oscilloscope

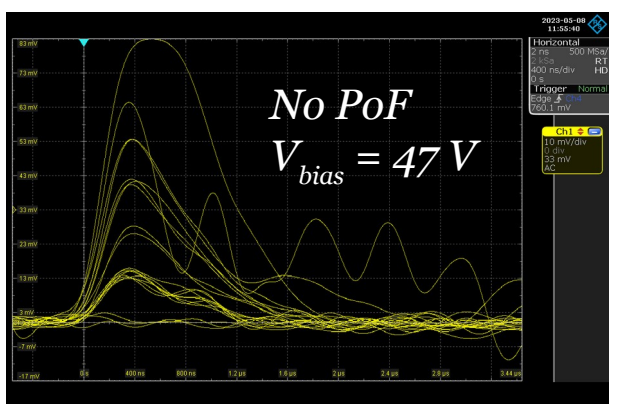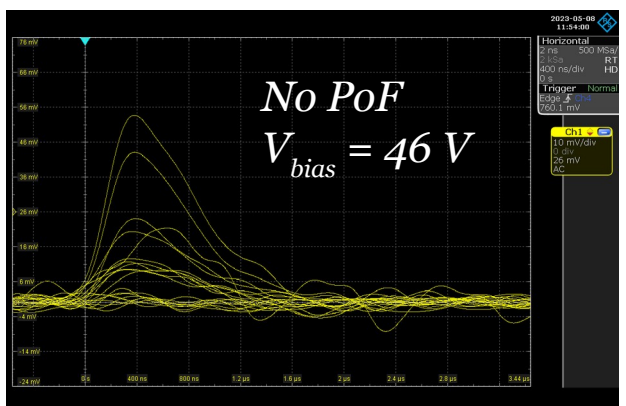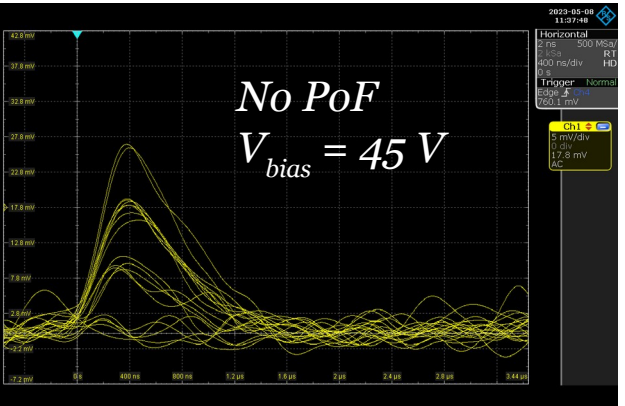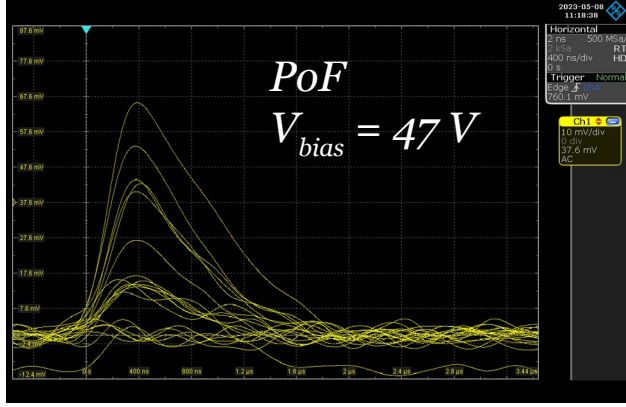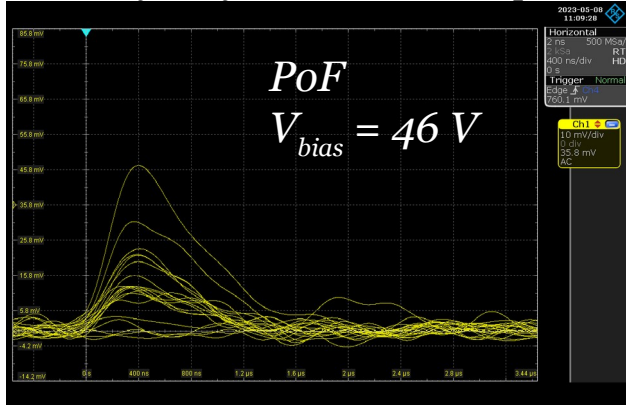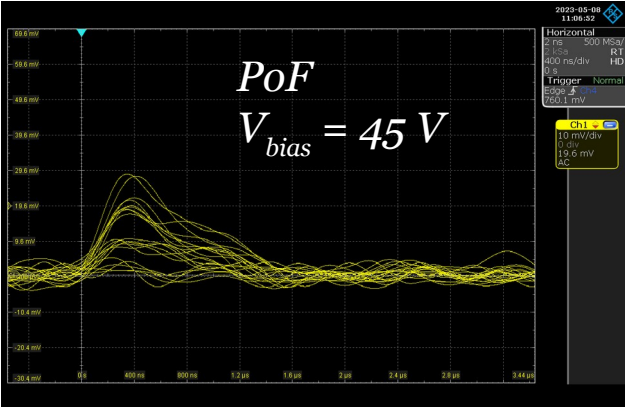


## Copper cable

*1 phe mean waveform*

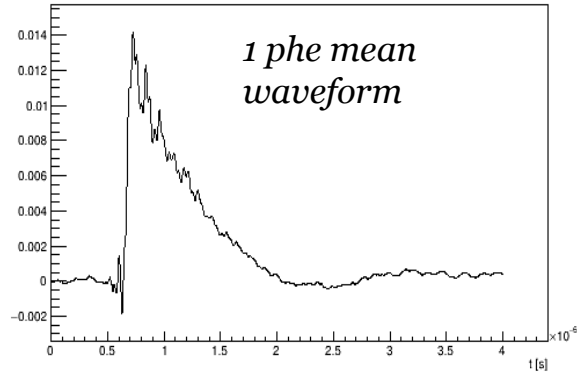


$$V_{\text{bias}} = 45 \text{ V} - 3 \text{ V ov}$$

**SNR = 7.830**

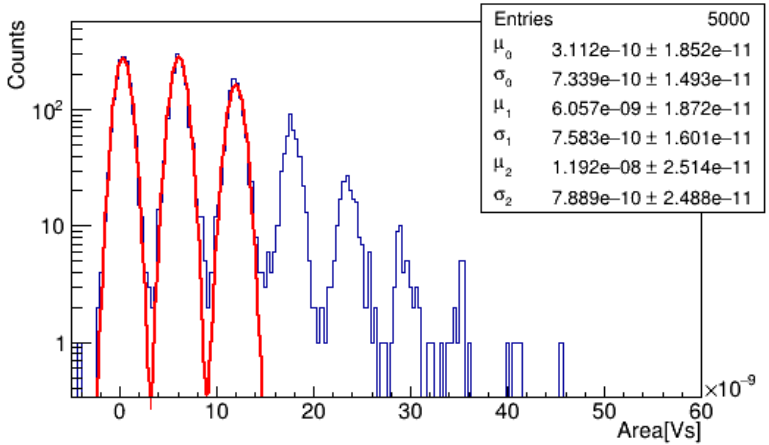

## PoF


*1 phe mean waveform*

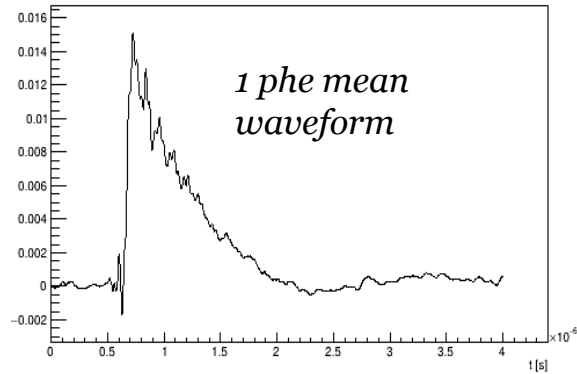

$$V_{\text{in laser}} = -2.97 \text{ V}$$


$$V_{\text{bias}} = 45 \text{ V} - 3 \text{ V ov}$$

**SNR = 7.520**

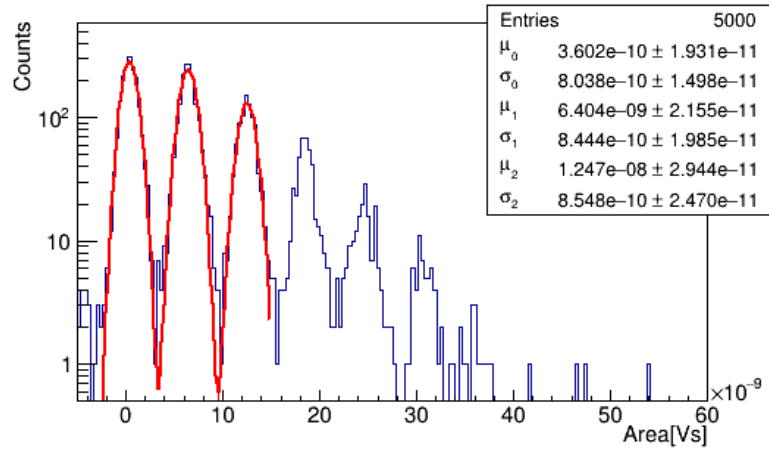


# Results

## Copper cable

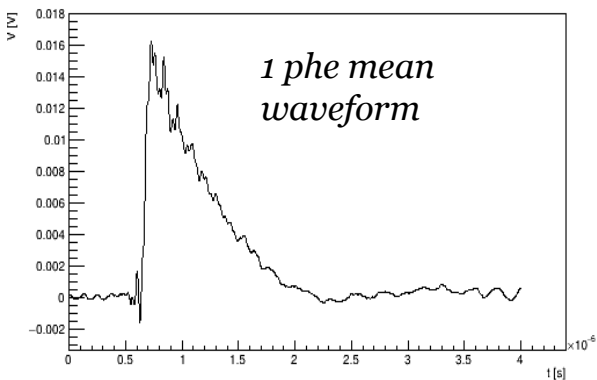


$$V_{\text{bias}} = 46 \text{ V} - 4 \text{ V ov}$$

$$\text{SNR} = 10.665$$

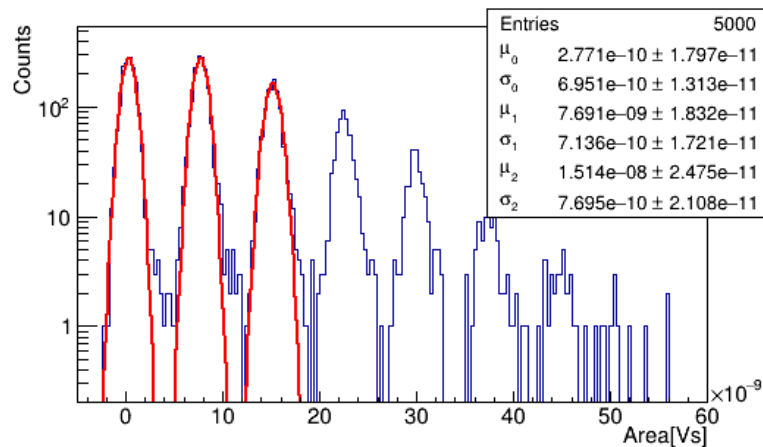


## PoF

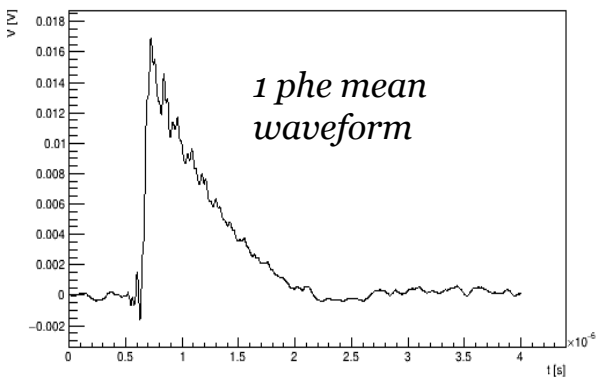


$$V_{\text{in laser}} = -2.83 \text{ V}$$

$$V_{\text{bias}} = 46 \text{ V} - 4 \text{ V ov}$$

$$\text{SNR} = 9.409$$

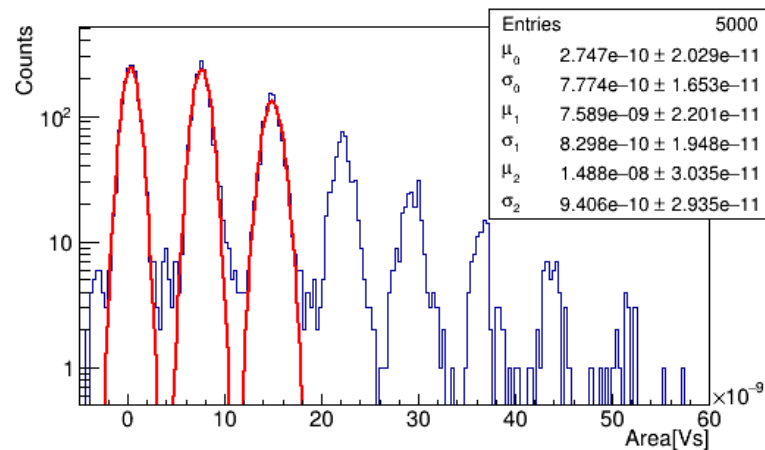


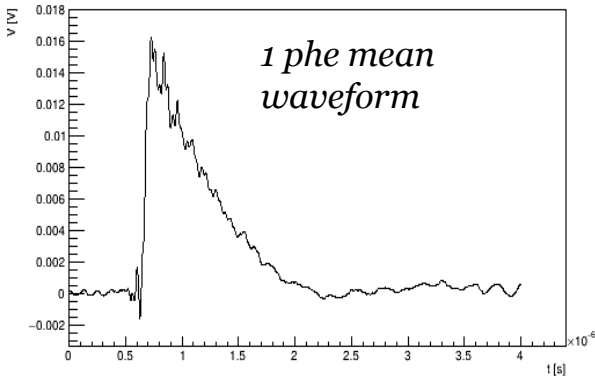


## Copper cable

$$V_{\text{bias}} = 47 \text{ V} - 5 \text{ V ov}$$

**SNR = 13.004**

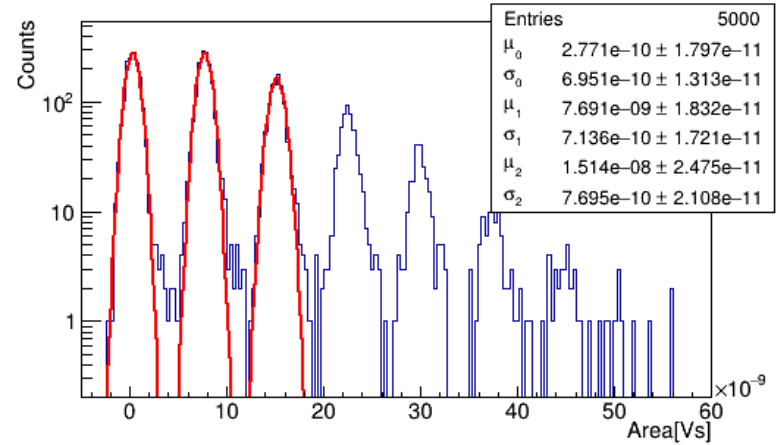


## PoF

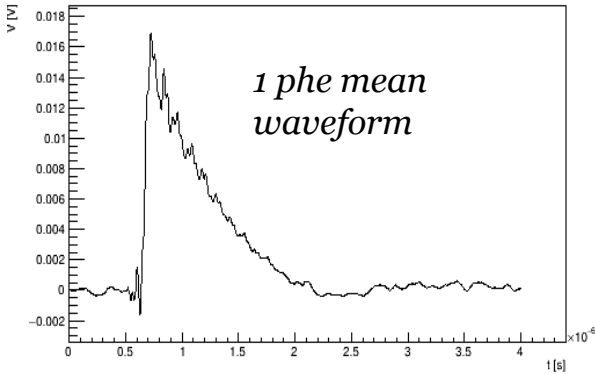


$$V_{\text{in laser}} = -2.61 \text{ V}$$
$$V_{\text{bias}} = 47 \text{ V} - 5 \text{ V ov}$$

**SNR = 11.070**

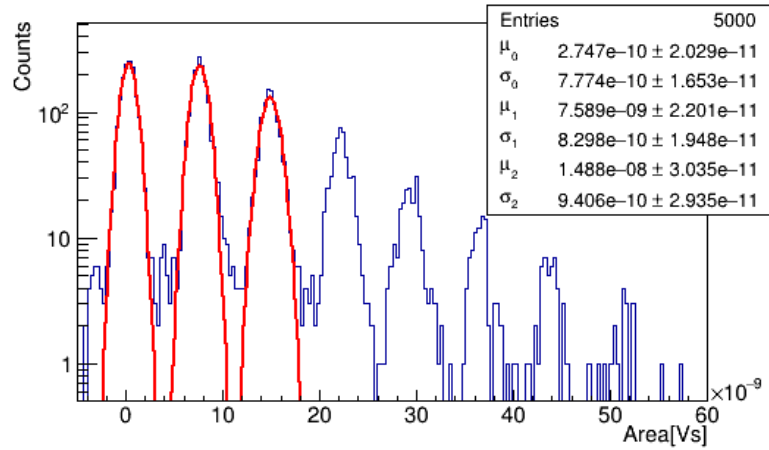

# DC-DC boost prototype test bench

- A matrix board is equipped with L1, D1, R1, C1:
  - **Load** is a **10 kΩ** resistor
- The Q1 (**NTF**) **transistor** can be changed to test all models
- **DC input** provided by a **linear supply** (AimTTi PL303QMD-P)
- The input current is monitored with a multimeter (HP 971A)
- The **control signal** is produced by a **Pattern Generator** (HP HP 81104A), High-level = 5 V, Low-Level = 0 V and rise/fall time = 3 ns with **100 kHz of period**.

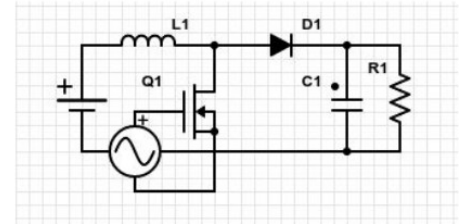

L1	10 mH
D1	BAV16W
C1	C0G 100 nF
R1	10 kΩ
Q1	NTF3055L108T1G

The system is tested at room and LN2 temperature, with different inputs (4V, 5V) and different duty cycle [0.1, 0.93].

- Output readout with a Lecroy HDO6104A oscilloscope.



# PDS - Cold electronics

- ❑ Used to collect the signals of 48 SiPMs of a supercell into a single readout channel.
- ❑ Each channel reads out 48 6x6 mm<sup>2</sup> SiPMs → 60 nF total input capacitance.
- ❑ 1 channel per SuperCell, 4 channels per module, 6000 channels in DUNE (1st module).
- ❑ Two-stage amplifier - SiGe bipolar transistor + fully differential op-amp.
- ❑ Low series noise is required → SiGe input transistor gives 0.37 nV/ $\sqrt{\text{Hz}}$  at cryo temperature.
- ❑ Low power consumption (2 mW/channel) to prevent boiling of LAr.

